


Supplemental figure 2

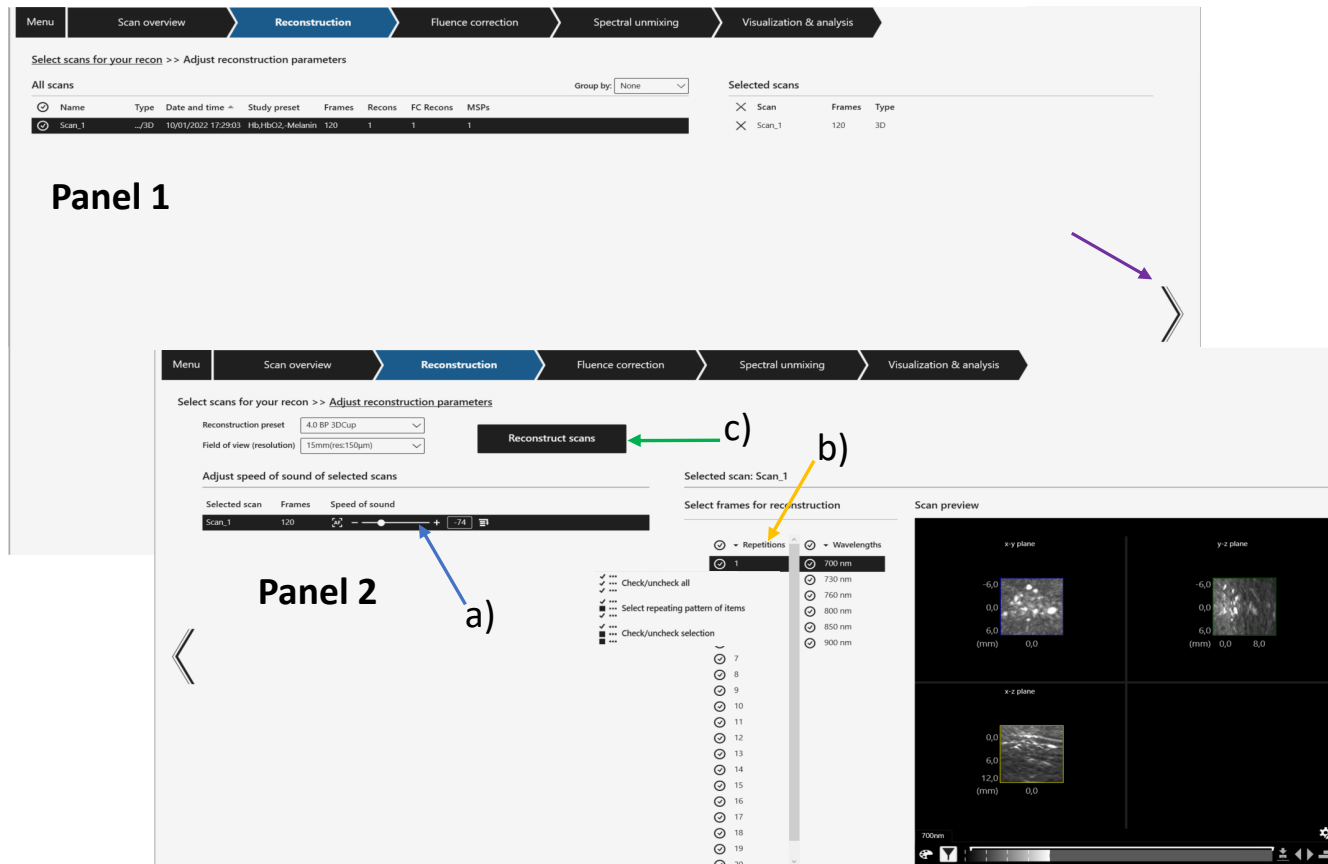

supplementary Figure 2: Reconstruction analysis workflow. Panel 1- Select the scan to be reconstructed and press the button in the right side of the screen (purple arrow). Panel 2 - Observe the speed of sound and adjust the slider to the best focus (blue arrow; a) adjusted focus displayed in the window right hand side; b) select repetitions to be analysed (yellow arrow); c) press the **reconstruct scans** button to proceed (green arrow). n