


Supplemental figure 4

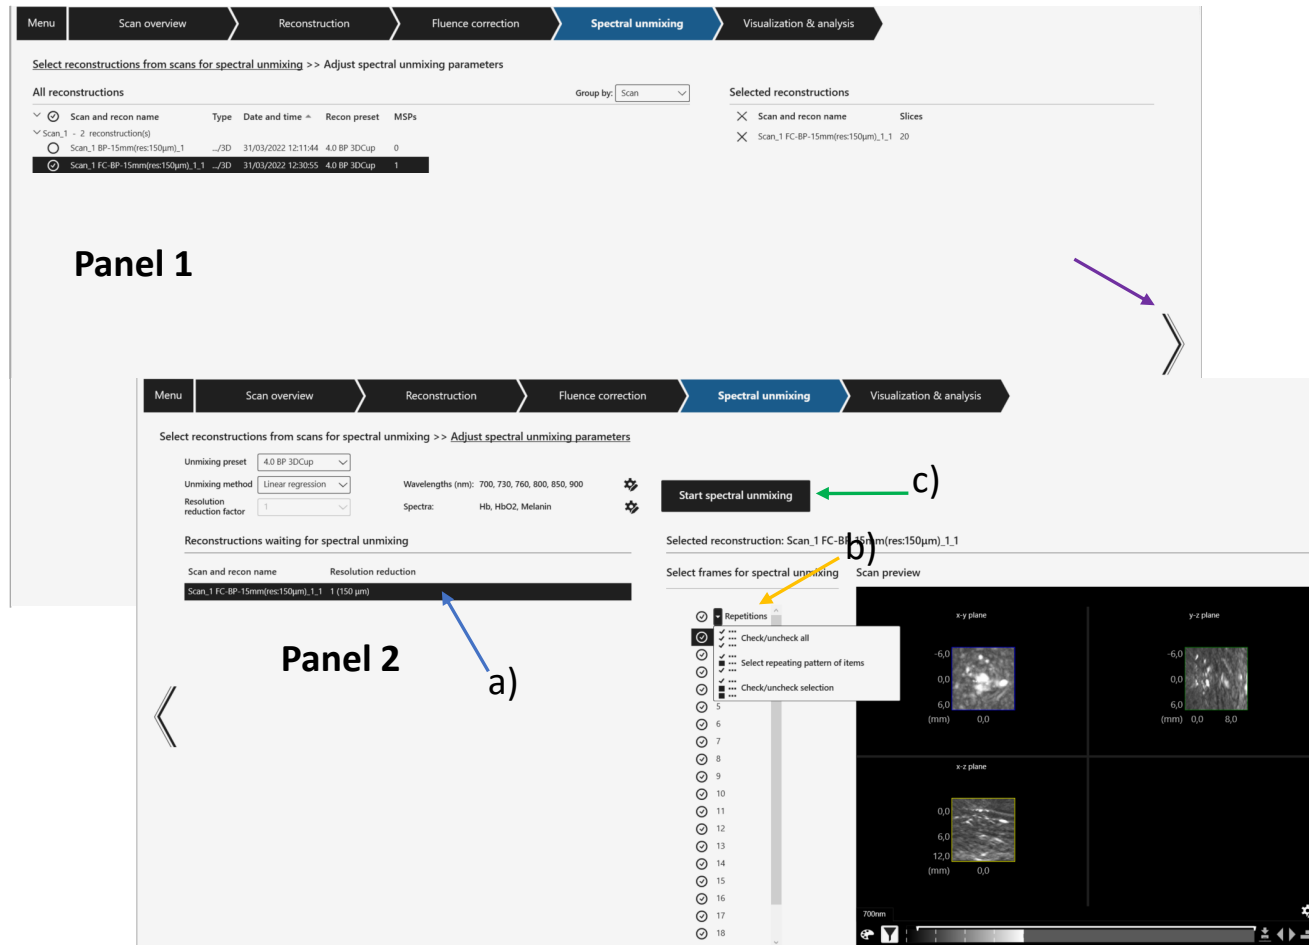

Supplementary Figure 4: Spectra unmixing panel

Workflow for spectral unmixing. Panel 1 - Select scans to unmix and press the button (right screen, purple arrow). Panel 2 a) select the scan to unmix (blue arrow) and a preview of the adjusted image will be displayed in the right hand side; b) Select the repetitions to unmix (yellow arrow); c) press the **Start spectral unmixing** to proceed (green arrow).