


Supplemental figure 5

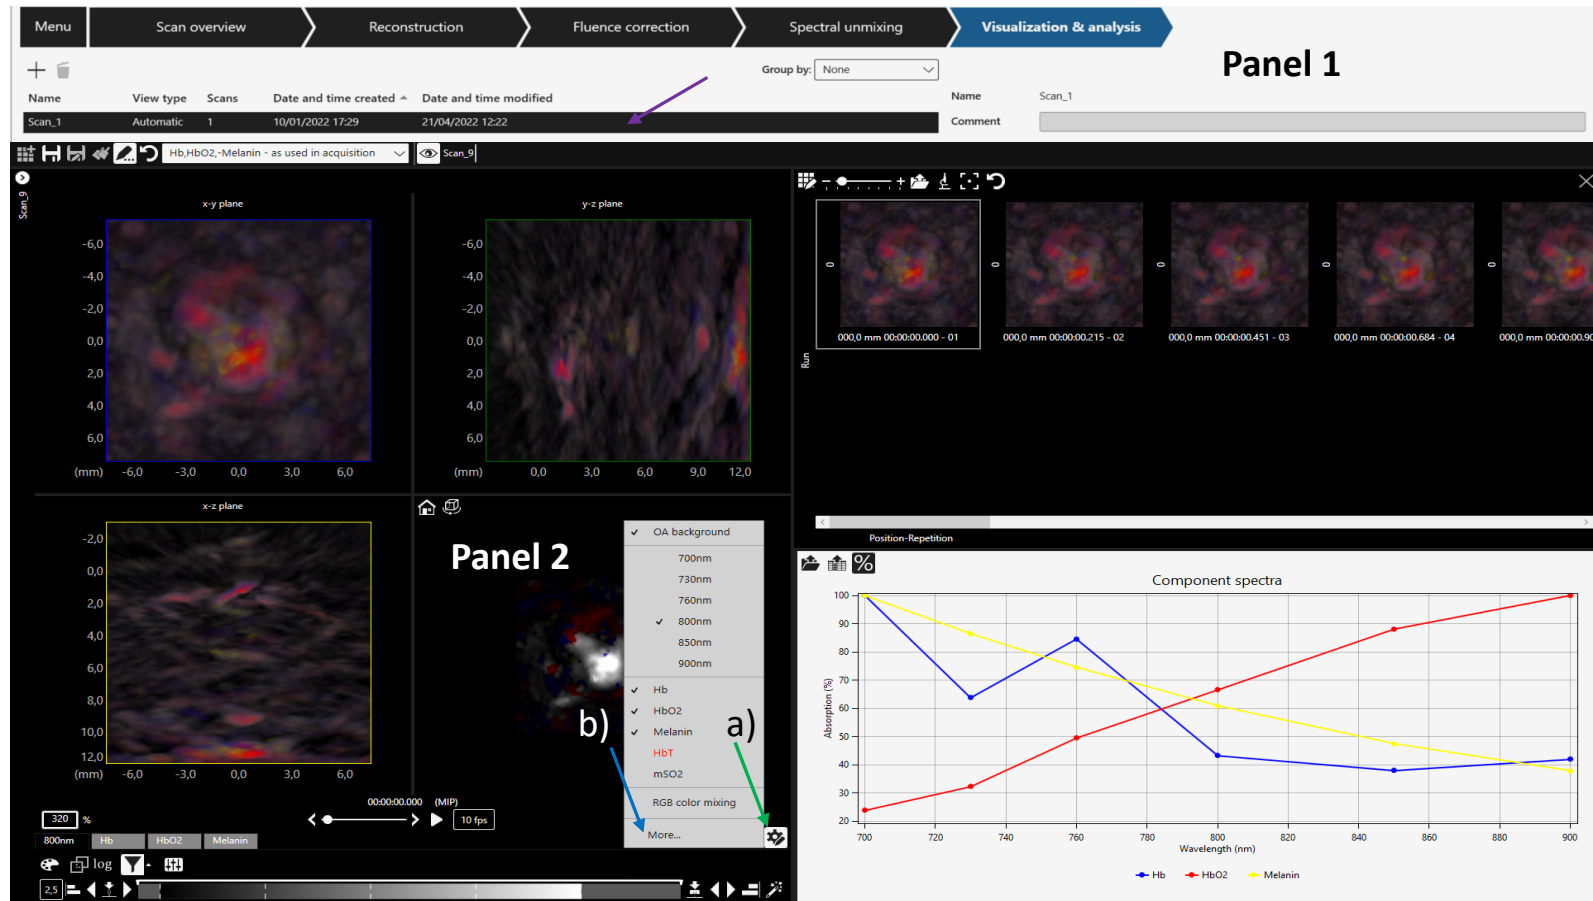

supplementary Figure 5: Visualisation panel and selection of chromophore colours.

Panel 1) Select scans to display with a double click (purple arrow); Panel 2) Acquired image in axis XY (blue square), XZ (yellow square) and YZ (green square); 2 a) Image analysis button showing acquired wavelengths; 2b) choose **More Image Control Options** in the top menu bar and activate the Max Intensity Projection icon; select **More** to edit channels' colours.