


- Connect
- Drift Correct
- Focus Assist
- Calibrate Focus
- Tag Images
- Review Session
- Close Session
- Diagnostic Report
- Settings
- Exit

01/17/2023 16:34:32.681
 Dose Rate: 0.3548 e⁻/Å²s
 Max Dose: 14.70 e⁻/Å²

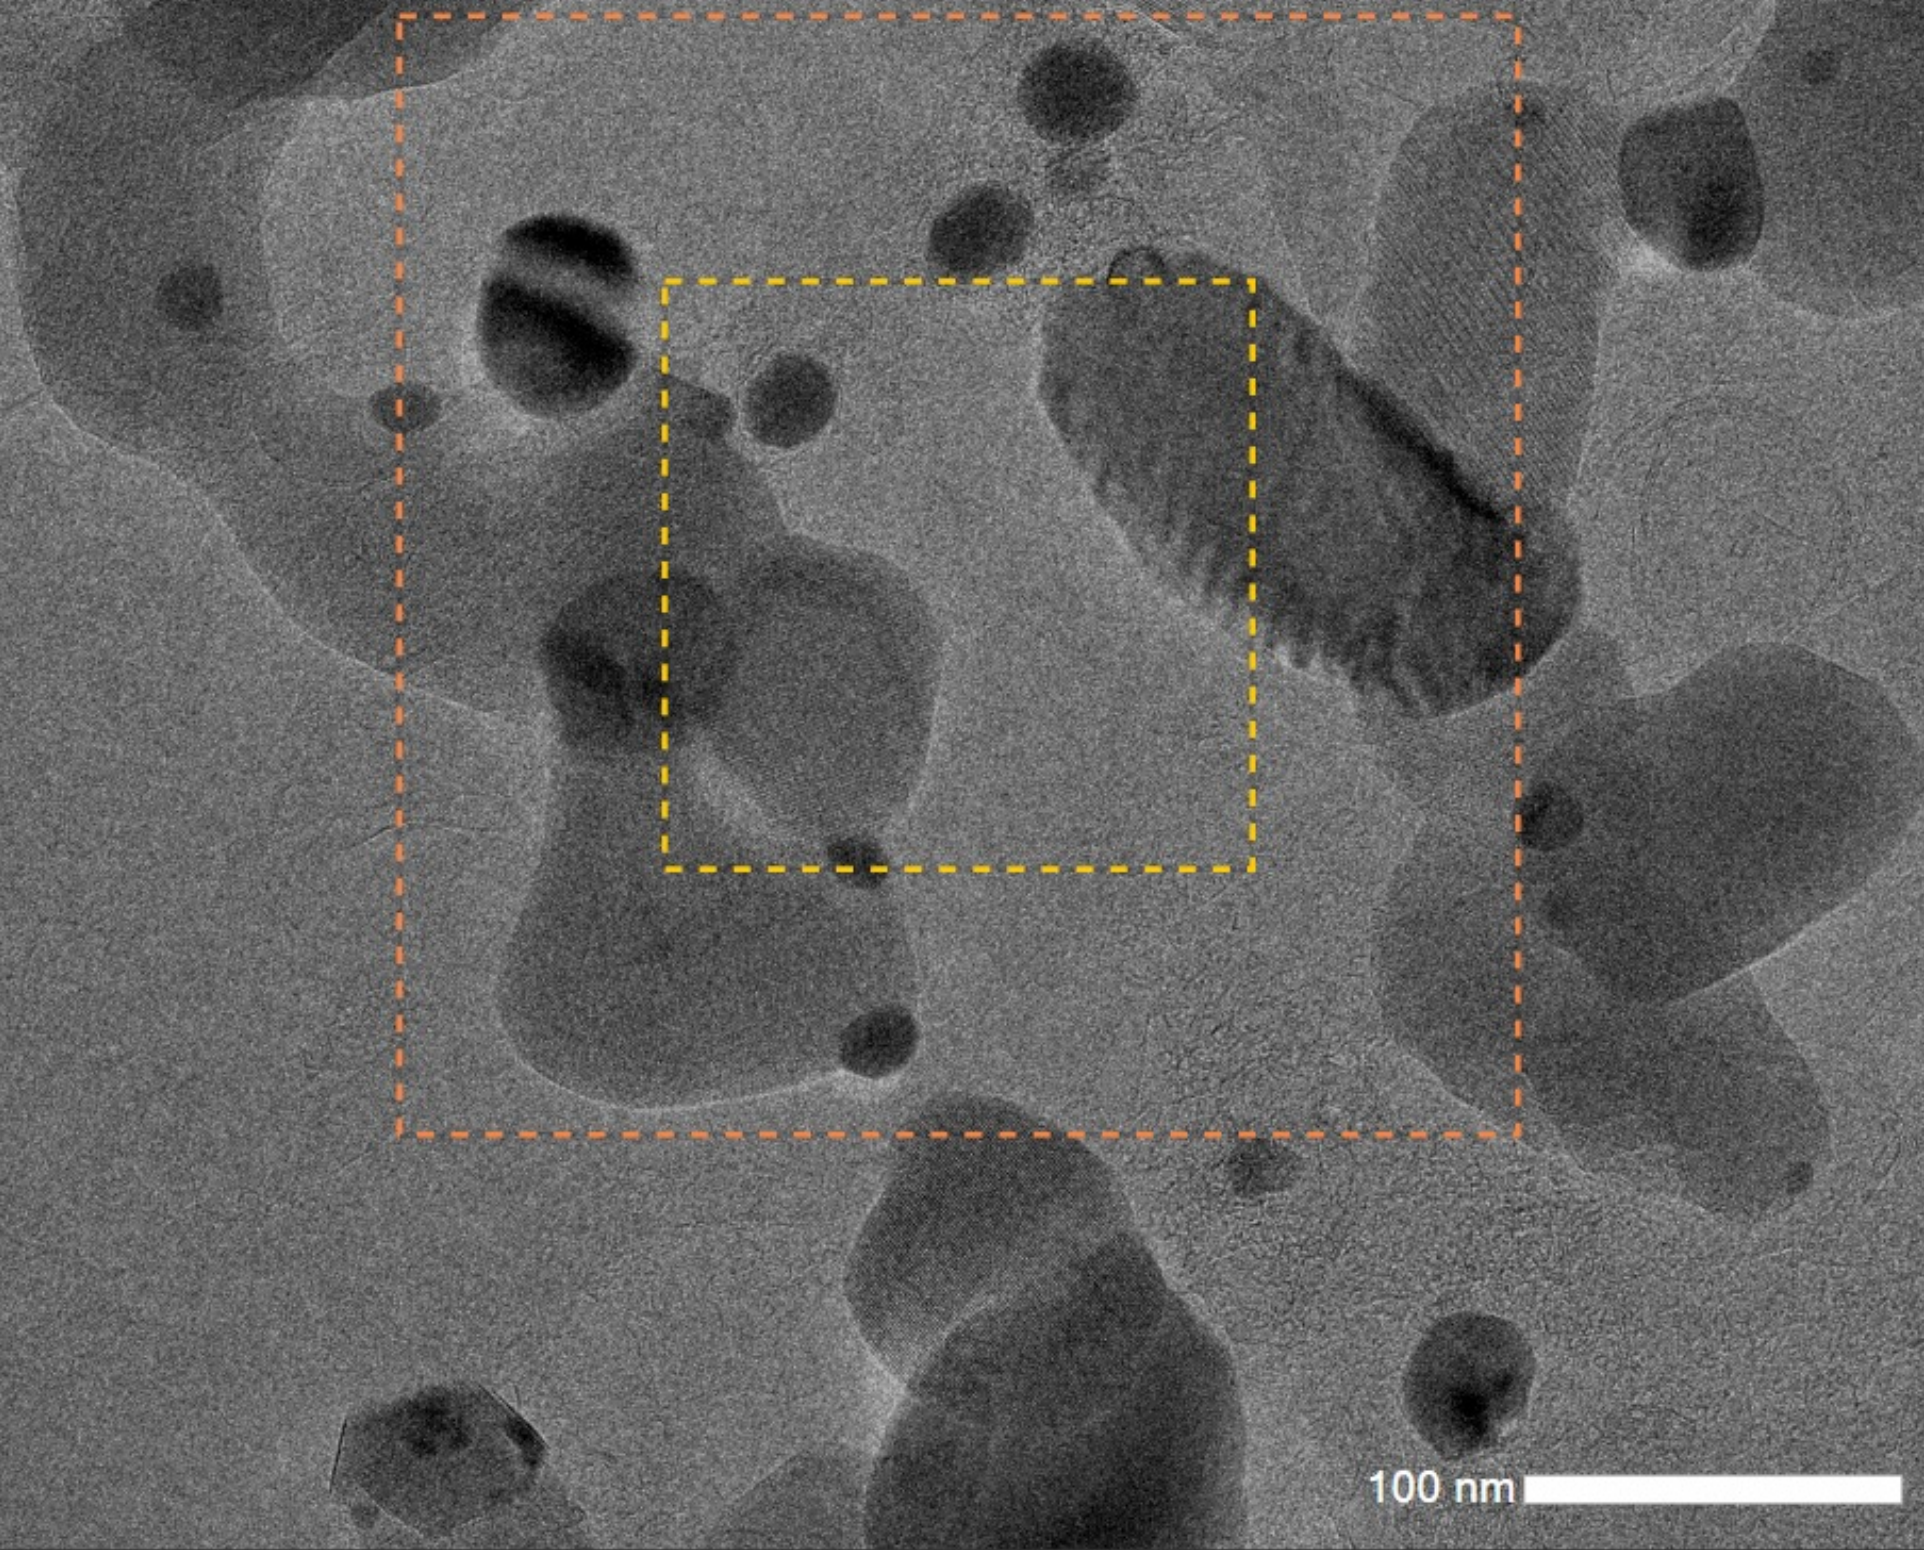

OTHER WORKFLOWS

Image Metadata

Image Analysis

Data View

Dose

Dose Calibration

Dose Management

Sample Management

Sample Type Default

Sample Type Name Default

Save

Delete

Low Dose Level 71.8422 e⁻/Å²

High Dose Level 192.7963 e⁻/Å²

High Dose Rate 12.7726 e⁻/Å²s

Dose Monitoring

Enable Dose Monitoring


Show Dose Layer

Show Position Uncertainty

Max Cumulative Dose (e⁻/Å²) 14.7009

Dose Rate (e⁻/Å²s) 0.3548

Set Dose Levels

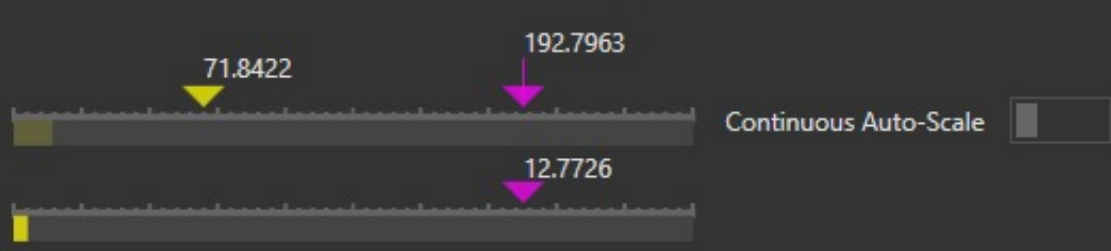

Dose Navigation

Service

Notifications

- 2023-01-17 16:33:09.277: Drift template updated
- 2023-01-17 16:33:11.627: Focus assist starting
- 2023-01-17 16:33:11.761: Focus assist started
- 2023-01-17 16:33:14.367: Focus assist stopped
- 2023-01-17 16:33:14.673: Drift correction stopped
- 2023-01-17 16:33:23.968: Drift correction started
- 2023-01-17 16:33:24.511: Focus assist starting
- 2023-01-17 16:33:24.752: Drift template updated
- 2023-01-17 16:33:25.248: Focus assist started